



Instruction for Use

Blood Collection with S-Monovette® for use with Roche Multiplate® Analyser

Blood Collection with S-Monovette® Hirudin and Vacuum Needle & Vacuum Holder

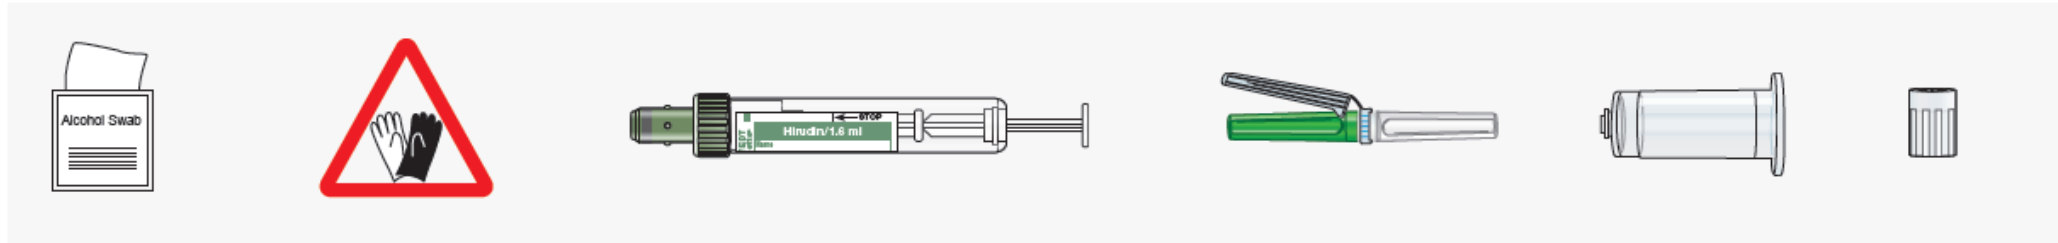

Vacuum method – Always a fresh vacuum

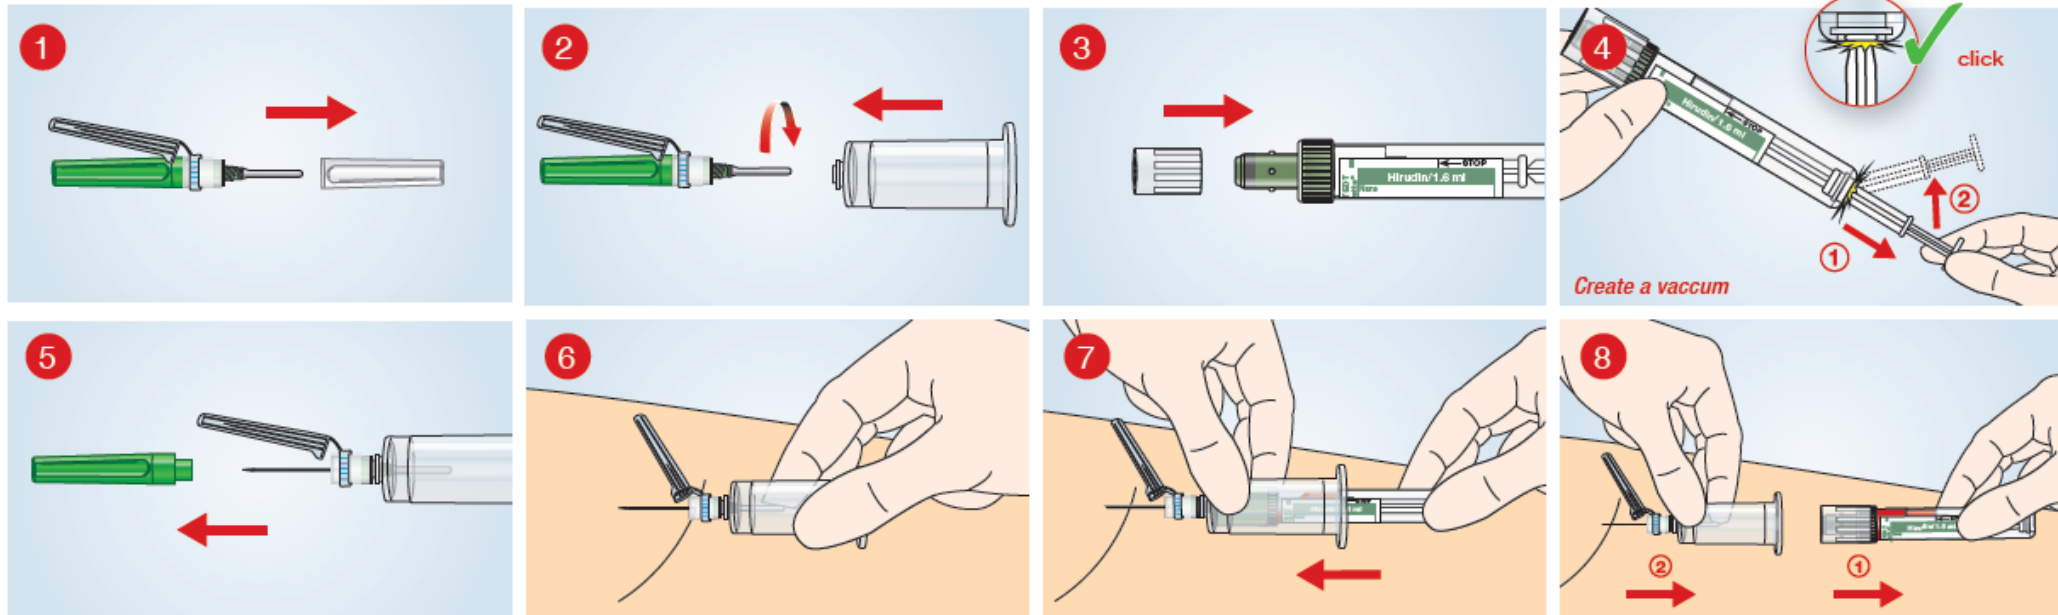

SARSTEDT AG & Co. KG
P.O. Box 12 20
D-51582 Nümbrecht
Phone +49 2293 305-0
Fax +49 2293 305-3992
export@sarstedt.com
www.sarstedt.com